

Eukaryotic Osteopontin (OPN) Instruction Manual

SFPA204Ra61

Rattus norvegicus (Rat)

Source	Eukaryotic expression
Host	293F cell
Endotoxin Level	<1.0EU per 1ug (determined by the LAL method)
Subcellular Location	Secreted
Predicted Molecular Mass	34.9kDa
Accurate Molecular Mass	35kDa(Analysis of differences refer to the manual)
Residues & Tags	Leu17~Asn317 with N-terminal His Tag
Buffer Formulation	20mM Tris, 150mM NaCl, pH8.0, containing 1mM EDTA, 1mM DTT, 5% Trehalose and Proclin300.
Traits	Freeze-dried powder
Purity	> 95%
Isoelectric Point	4.3
Applications	Positive Control; Immunogen; SDS-PAGE; WB.

SEQUENCE

```
LPVK VAEFGSSEEK AHYSKHSDAV ATWLKPDPSQ  
KQNLLAPQNS VSSEETDDFK QETLPSNSNE SHDHMDDDDD DDDGDHAES  
EDSVNSDESD ESHHSDESDE SFTASTQADV LTPIAPTVDV PDGRGDSLAY  
GLRSKRSRFP VSDEQYPDAT DEDLTSRMKS QESDEAIKVI PVAQRSLVPS  
DQDSNGKTSH ESSQLDEPSV ETHSLEQSKE YKQRASHEST EQSDAIDSAE  
KPDAIDSAER SDAIDSQASS KASLEHQSHE FHSHEDKLVL DPKSKEDDRY  
LKFRISHELE SSSSEVN
```

```
LPVK VAEFGSSEEK AHYSKHSDAV ATWLKPDPSQ  
KQNLLAPQNS VSSEETDDFK QETLPSNSNE SHDHMDDDDD DDDGDHAES  
EDSVNSDESD ESHHSDESDE SFTASTQADV LTPIAPTVDV PDGRGDSLAY  
GLRSKRSRFP VSDEQYPDAT DEDLTSRMKS QESDEAIKVI PVAQRSLVPS  
DQDSNGKTSH ESSQLDEPSV ETHSLEQSKE YKQRASHEST EQSDAIDSAE  
KPDAIDSAER SDAIDSQASS KASLEHQSHE FHSHEDKLVL DPKSKEDDRY  
LKFRISHELE SSSSEVN
```

USAGE

Reconstitute in 20mM Tris, 150mM NaCl (pH8.0) to a concentration of 0.1-1.0 mg/mL. Do not vortex.

STORAGE

Avoid repeated freeze/thaw cycles. Store at 2-8°C for one month. Aliquot and store at -80°C for 12 months.

STABILITY

The thermal stability is described by the loss rate. The loss rate was determined by accelerated thermal degradation test, that is, incubate the protein at 37°C for 48h, and no obvious degradation and precipitation were observed. The loss rate is less than 5% within the expiration date under appropriate storage condition.

Image

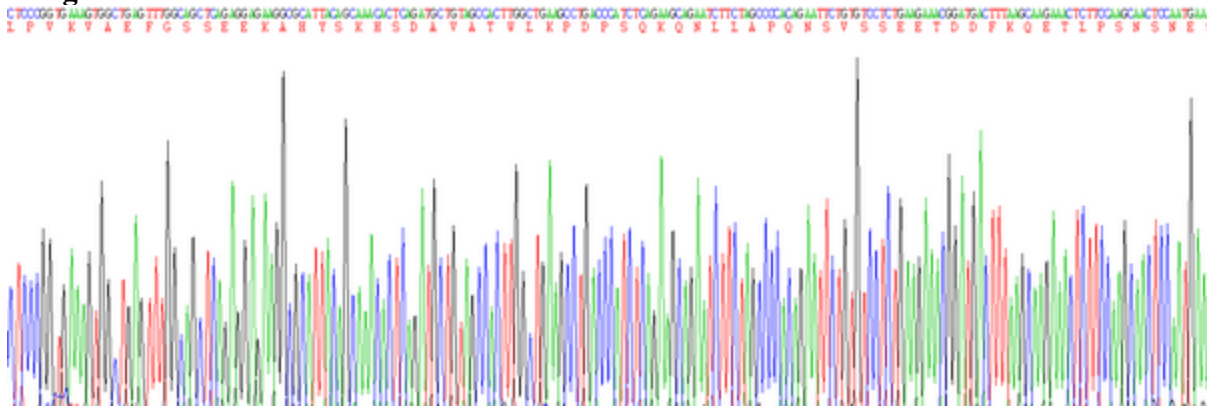


Figure. SDS-PAGE

[IMPORTANT NOTE]

The kit is designed for research use only, we will not be responsible for any issue if the kit was used in clinical diagnostic or any other procedures.