

# Recombinant Cluster Of Differentiation 14 (CD14) Instruction Manual

## SIPA163Hu02

**Homo sapiens (Human)**

<b>Source</b>	Prokaryotic expression
<b>Host</b>	E.coli
<b>Endotoxin Level</b>	<1.0EU per 1µg (determined by the LAL method)
<b>Subcellular Location</b>	Membrane, Secreted
<b>Predicted Molecular Mass</b>	42.9kDa
<b>Accurate Molecular Mass</b>	50kDa(Analysis of differences refer to the manual)
<b>Residues &amp; Tags</b>	Thr20~Leu368 with N-terminal His Tag
<b>Buffer Formulation</b>	20mM Tris, 150mM NaCl, pH8.0, containing 1mM EDTA, 1mM DTT, 0.01% SKL, 5% Trehalose and Proclin300.
<b>Traits</b>	Freeze-dried powder
<b>Purity</b>	> 90%
<b>Isoelectric Point</b>	5.7
<b>Applications</b>	Positive Control; Immunogen; SDS-PAGE; WB.

## SEQUENCE

```
          T TPEPCELDDE DFRVCVNFSE PQPDWSEAFQ  
CVSAVEVEIH AGGLNLEPFL KRVDADADPR QYADTVKALR VRRLTVGAAQ  
VPAQLLVGAL RVLAYSRLKE LTLEDLKITG TMPPLPLEAT GLALSSLRLR  
NVSATGRSW LAELQQWLKP GLKVLSIAQA HSPAFSCEQV RAFPALTSLD  
LSDNPGLGER GLMAALCPHK FPAIQNLALR NTGMETPTGV CAALAAAGVQ  
PHSLDLSHNS LRATVNPSAP RCMWSSALNS LNLSFAGLEQ VPKGLPAKLR  
VLDLSCNRLN RAPQPDELPE VDNLTLDGNP FLVPGTALPH EGSMN SGVVP  
ACARSTLSVG VSGTLVLL
```

## USAGE

Reconstitute in ddH<sub>2</sub>O to a concentration of 0.1-1.0 mg/mL. Do not vortex.

## STORAGE

Avoid repeated freeze/thaw cycles. Store at 2-8°C for one month. Aliquot and store at -80°C for 12 months.

## STABILITY

The thermal stability is described by the loss rate. The loss rate was determined by accelerated thermal degradation test, that is, incubate the protein at 37°C for 48h, and no obvious degradation and precipitation were observed. The loss rate is less than 5% within the expiration date under appropriate storage condition.

## Image

gaaTTcaccagocagAACCTTGtGAGCTGGAGGATGaaGATTCCGCTGCGTCTGCACCTTCCTCGAACCTCAgCCCGACtGGTCCGaaGCCTTCCAGTGTGTGTCTGCAGTgAGGTGGAGATCCATGCGGCGGTCTCAAOCTAGAGCCGTTTCTAAAAGCGCG

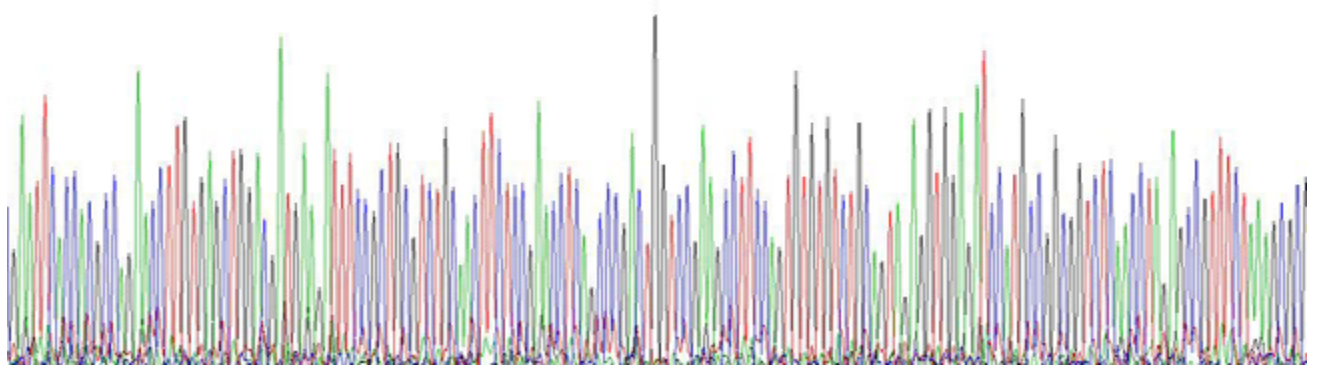


Figure. SDS-PAGE

## **[IMPORTANT NOTE]**

The kit is designed for research use only, we will not be responsible for any issue if the kit was used in clinical diagnostic or any other procedures.