

# Recombinant Sirtuin 2 (SIRT2) Instruction Manual

**SIPA774Hu01**

**Homo sapiens (Human)**

|                                 |   |
|---------------------------------|---|
| <b>Source</b>                   | Prokaryotic expression  |
| <b>Host</b>                     | E.coli  |
| <b>Endotoxin Level</b>          | <1.0EU per 1µg (determined by the LAL method)   |
| <b>Subcellular Location</b>     | Cytoplasm   |
| <b>Predicted Molecular Mass</b> | 34.8kDa   |
| <b>Accurate Molecular Mass</b>  | 33kDa(Analysis of differences refer to the manual)  |
| <b>Residues &amp; Tags</b>      | Glu65~Glu340 with N-terminal His Tag  |
| <b>Buffer Formulation</b>       | 20mM Tris, 150mM NaCl, pH8.0, containing 1mM EDTA, 1mM DTT, 0.01% SKL, 5% Trehalose and Proclin300. |
| <b>Traits</b>                   | Freeze-dried powder   |
| <b>Purity</b>                   | > 90%   |
| <b>Isoelectric Point</b>        | 6.7   |
| <b>Applications</b>             | Positive Control; Immunogen; SDS-PAGE; WB.  |

## SEQUENCE

```
EGVARY MQSERCRRVI CLVGAGISTS AGIPDFRSPS  
TGLYDNLEKY HLPYPEAIFE ISYFKKHPEP FFALAKELYP GQFKPTICHY  
FMRLKDKGL LLRCYTQNIID TLERIAGLEQ EDLVEAHGTF YTSHCVSASC  
RHEYPLSWMK EKIFSEVTPK CEDCQSLVKP DIVFFGESLP ARFFSCMQSD  
FLKVDLLLVM GTSLQVQPFA SLISKAPLST PRLINKEKA GQSDPFLGMI  
MGLGGGMDFD SKKAYRDVAW LGECDQGCLA LAELLGWKKE
```

## USAGE

Reconstitute in 20mM Tris, 150mM NaCl (pH8.0) to a concentration of 0.1-1.0 mg/mL.  
Do not vortex.

## STORAGE

Avoid repeated freeze/thaw cycles. Store at 2-8°C for one month. Aliquot and store at -80°C for 12 months.

## **STABILITY**

The thermal stability is described by the loss rate. The loss rate was determined by accelerated thermal degradation test, that is, incubate the protein at 37°C for 48h, and no obvious degradation and precipitation were observed. The loss rate is less than 5% within the expiration date under appropriate storage condition.

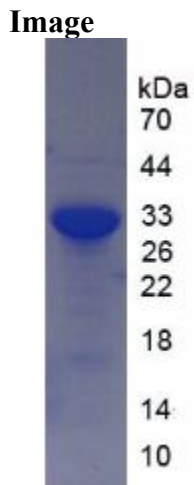


Figure. SDS-PAGE

## **[IMPORTANT NOTE]**

The kit is designed for research use only, we will not be responsible for any issue if the kit was used in clinical diagnostic or any other procedures.