

# Recombinant Aspartate Aminotransferase 2 (AST2) Instruction Manual

**SIPD565Hu01**

**Homo sapiens (Human)**

<b>Source</b>	Prokaryotic expression
<b>Host</b>	E.coli
<b>Endotoxin Level</b>	<1.0EU per 1µg (determined by the LAL method)
<b>Subcellular Location</b>	Secreted
<b>Predicted Molecular Mass</b>	46.0kDa
<b>Accurate Molecular Mass</b>	46kDa(Analysis of differences refer to the manual)
<b>Residues &amp; Tags</b>	Ser30~Lys430 with N-terminal His Tag
<b>Buffer Formulation</b>	20mM Tris, 150mM NaCl, pH8.0, containing 1mM EDTA, 1mM DTT, 0.01% SKL, 5% Trehalose and Proclin300.
<b>Traits</b>	Freeze-dried powder
<b>Purity</b>	> 95%
<b>Isoelectric Point</b>	8.9
<b>Applications</b>	Positive Control; Immunogen; SDS-PAGE; WB.

## SEQUENCE

```

                                     S  SWWTHVEMGP  PDPILGVTEA
FKRDTNSKMM  NLGVGAYRDD  NGKPYVLPSV  RKAEAQIAAK  NLDKEYLPIG
GLAEFCKASA  ELALGENSEV  LKSGRFVTVQ  TISGTGALRI  GASFLQRFFK
FSRDVFLPKP  TWGNHTPIFR  DAGMQLQGYR  YYDPKTCGFD  FTGAVEDISK
IPEQSVLLLLH  ACAHNPTGVD  PRPEQWKEIA  TVVKKRNLFA  FFDMAYQGFA
SGDGDKDAWA  VRHFIEQGIN  VCLCQSYAKN  MGLYGERVGA  FTMVCKDADE
AKRVESQLKI  LIRPMSYNNP  LNGARIAAAI  LNTPLRLKQW  LQEVKVMADR
IIGMRTLQVLS  NLKKEGSTHN  WQHITDQIGM  FCFTGLKPEQ  VERLIKEFSI
YMTKDGRISV  AGVTSSNVGY  LAHAIHQVTK
```

## USAGE

Reconstitute in 20mM Tris, 150mM NaCl (pH8.0) to a concentration of 0.1-1.0 mg/mL.  
Do not vortex.

## STORAGE

Avoid repeated freeze/thaw cycles. Store at 2-8°C for one month. Aliquot and store at -80°C for 12 months.

## STABILITY

The thermal stability is described by the loss rate. The loss rate was determined by accelerated thermal degradation test, that is, incubate the protein at 37°C for 48h, and no obvious degradation and precipitation were observed. The loss rate is less than 5% within the expiration date under appropriate storage condition.

## Image

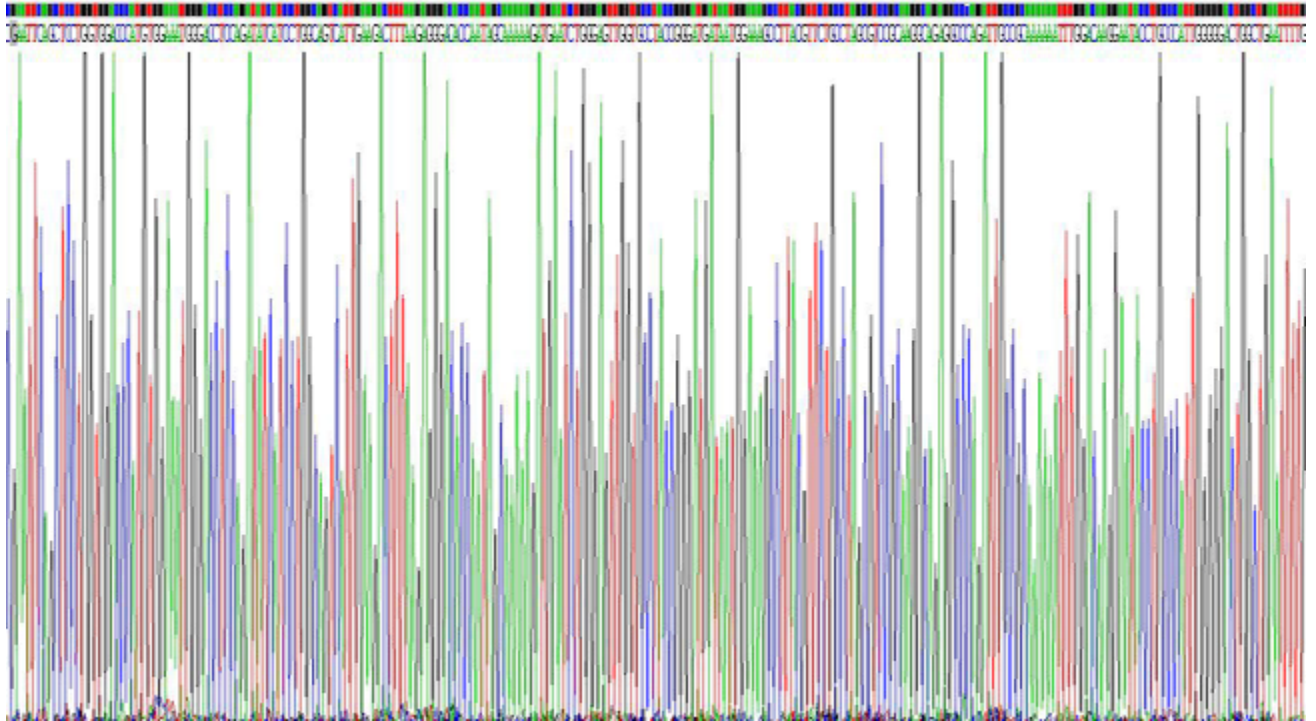


Figure. SDS-PAGE

## **[IMPORTANT NOTE]**

The kit is designed for research use only, we will not be responsible for any issue if the kit was used in clinical diagnostic or any other procedures.