

# Recombinant Glutamate Receptor, Ionotropic, N-Methyl-D-Aspartate 2D (GRIN2D) Instruction Manual

**SIPE183Hu01**

**Homo sapiens (Human)**

<b>Source</b>	Prokaryotic expression
<b>Host</b>	E.coli
<b>Endotoxin Level</b>	<1.0EU per 1µg (determined by the LAL method)
<b>Subcellular Location</b>	Membrane
<b>Predicted Molecular Mass</b>	63.7kDa
<b>Accurate Molecular Mass</b>	64kDa(Analysis of differences refer to the manual)
<b>Residues &amp; Tags</b>	Phe28~Ala584 with N-terminal His Tag
<b>Buffer Formulation</b>	20mM Tris, 150mM NaCl, pH8.0, containing 1mM EDTA, 1mM DTT, 0.01% SKL, 5% Trehalose and Proclin300.
<b>Traits</b>	Freeze-dried powder
<b>Purity</b>	> 90%
<b>Isoelectric Point</b>	5.7
<b>Applications</b>	Positive Control; Immunogen; SDS-PAGE; WB.

## SEQUENCE

```
FPE EAPGPGGAGG PGGGLGGARP
LNVALVFSGP AYAAEAARLG PAVAAAVRSP GLDVRPVALV LNGSDPRSLV
LQLCDLLSGL RVHGVPFEDD SRAPAVAPIL DFLSAQTSPLP IVAVHGGAAL
VLTPKEKGST FLQLGSSTEQ QLQVIFEVLE EYDWTSEFVAV TTRAPGHRAF
LSYIEVLTDG SLVGWEHRGA LTLDPGAGEA VLSAQLRSVS AQIRLLFCAR
EEAEPVFRAA EEAGLTGSGY VWFVGPQLA GGGGSGAPGE PPLLPGGAPL
PAGLFAVRSA GWRDDLARRV AAGVAVVARG AQALLRDYGF LPELGHDCRA
QNRTHRGESL HRYFMNITWD NRDYSFNEDG FLVNPSLVVI SLTRDRTWEV
VGSWEQQTLR LKYPLWSRYG RFLQPVDDTQ HLTVATLEER PFVIVEPADP
ISGTCIRDSV PCRSQNLNRTH SPPPDAPRPE KRCKGFCID ILKRLAHTIG
FSYDLYLVTN GKHGKKIDGV WNGMIGEVFY QRADMAIGSL TINEERSEIV
DFSVPFVETG ISVMVARSNG TVSPSAFLEP YSPA
```

## USAGE

Reconstitute in 20mM Tris, 150mM NaCl (pH8.0) to a concentration of 0.1-1.0 mg/mL. Do not vortex.

## STORAGE

Avoid repeated freeze/thaw cycles. Store at 2-8°C for one month. Aliquot and store at -80°C for 12 months.

## STABILITY

The thermal stability is described by the loss rate. The loss rate was determined by accelerated thermal degradation test, that is, incubate the protein at 37°C for 48h, and no obvious degradation and precipitation were observed. The loss rate is less than 5% within the expiration date under appropriate storage condition.

## Image

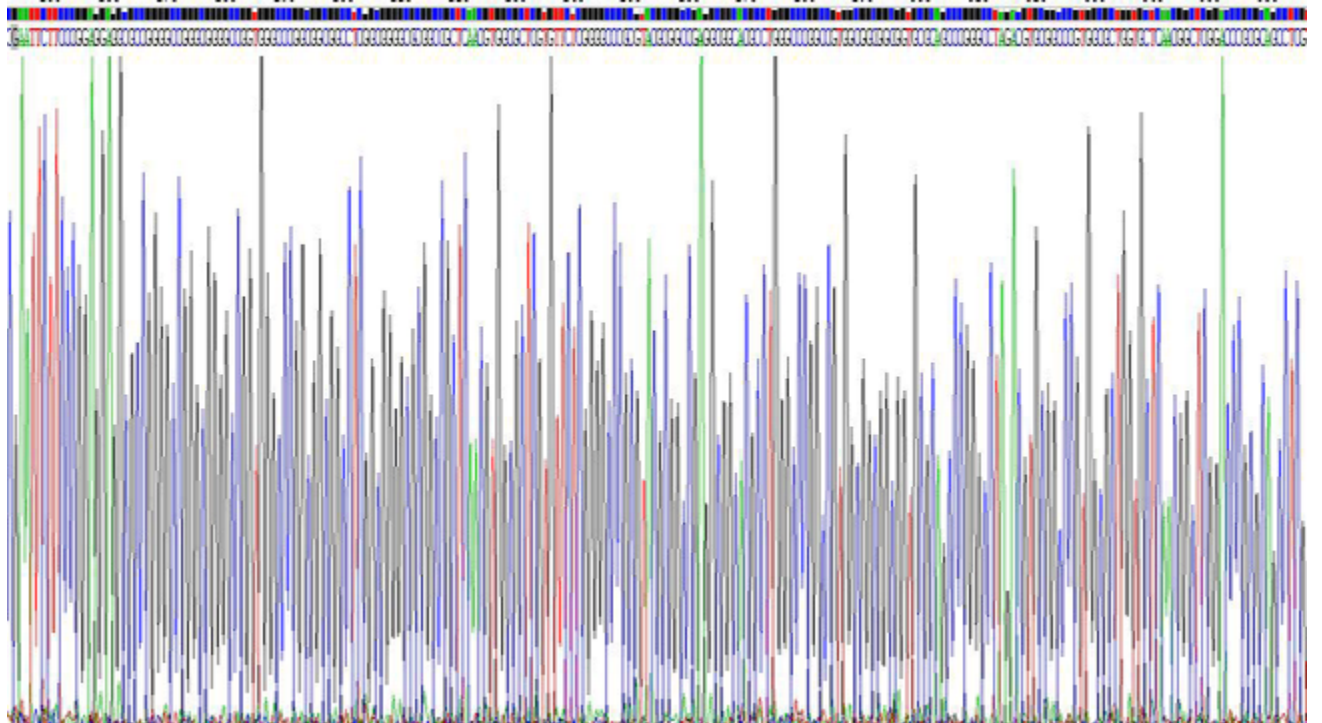


Figure. SDS-PAGE

**[IMPORTANT NOTE]**

The kit is designed for research use only, we will not be responsible for any issue if the kit was used in clinical diagnostic or any other procedures.